

# TD-450

## PRP centrifuge


Specifically for beauty hospital, Suitable for autologous fat transplantation surgery and autologous blood to extract for PRP cosmetic surgery.

### Features:

- Use of 10ml、20ml、50ml Syringe, 10ml Vacutainer and PRP accessory.
- Frequency conversion motor driving and maintenance-free, without pollution.
- Micro-computer control, digital display.
- Electronic lid locks and All-steel body.
- RCF can be directly set up and display, without RPM / RCF translated.
- The rotors and the accessories can be disinfected under high temperature and high pressure.

### Technical Parameters

Max Speed	4 500 r/min
Max RCF	3 380 Xg
Max Capacity	6X50ml Syringe
Speed accuracy	±20 r/min
Timer range	1-99 min/inching
Motor	frequency conversion motor
Noise	≤60dB(A)
Power	AC 220V 50HZ 10A
Dimension	550×450×365(L×W×H) mm
Weight	40 kg

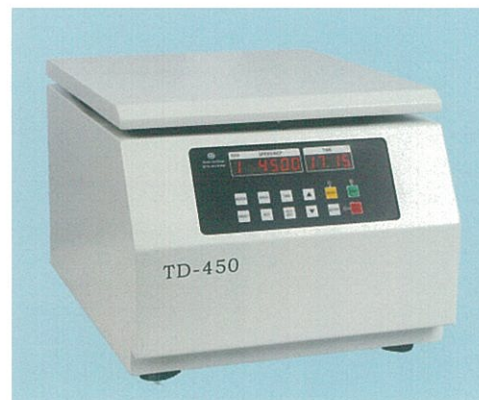

### Rotor Technical Data

Rotor	Capacity	Max Speed	Max RCF
NO.1 swing-out rotor	16x10 ml Syringe	4 000 rpm	3 000 Xg
NO.2 swing-out rotor	8x20 ml Syringe	4 000 rpm	3 100 Xg
NO.3 swing-out rotor	4x50 ml PRP accessories/Syringe	4 000 rpm	3 280 Xg
NO.4 swing-out rotor	24x10 ml blood collection tube	4 000 rpm	2 890 Xg
NO.5 angle rotor	6x50 ml Syringe	4 500 rpm	3 020 Xg

